

# Manual Torque Wrench Prosthetic

## Quick guide

This quick guide does not replace the instructions for use (IFU). For correct handling and torque specifications, see the instructions for use included with the individual product.

To ensure prostheses remain secured during daily patient use, tighten abutment and prosthetic screws to the recommended torque specifications.

## Instructions for use

The Manual Torque Wrench is a convenient tool for achieving the desired torque. It is easy to use, with a scale clearly indicating the two most common torque measurements, 15 Ncm and 35 Ncm.

### Step 1 – Assembly

Assemble the Manual Torque Wrench by inserting the screwdriver.

### Step 2 – Tightening



To tighten a screw, adjust the direction indicator so that the arrow is pointing toward the lever arm and rotate clockwise.

### Step 3 – Loosening

To loosen a screw, adjust the direction indicator so that the arrow is pointing away from the lever arm and rotate counterclockwise.







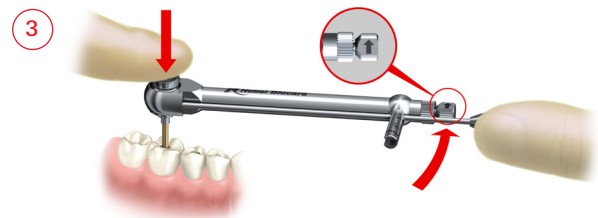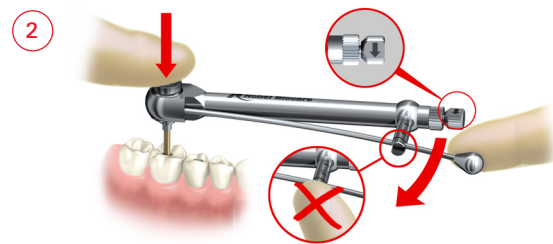














**Warning:** Using the wrench body instead of the lever arm may result in excessive torque being transferred to the screw and/or implant site.

**Note:** For prosthetic tightening, do not use the Manual Torque Wrench Surgical with the surgical adapter. The surgical manual torque wrench is intended for surgical use. However, a prosthetic adapter can be purchased and used together with the handle of a surgical manual torque wrench, thus turning it into a prosthetic manual torque wrench.



See reverse side for prosthetic component torque guide.

Prosthetic component torque guide

<p>Plastic Temporary Abutment Plastic Temporary Coping Healing Abutment Healing Cap</p>					<p>By hand</p>	
<p>Prosthetic Screws for final restorations Titanium Temporary Coping</p>					 <p>15 Ncm</p>	
<p>Ball Abutment 17° Multi-unit Abutment 30° Multi-unit Abutment</p>						
<p>Abutments for NobelActive® 3.0</p>  <p>Max 15 Ncm</p>						
<p>All other abutments for Nobel Biocare implant systems</p>						 <p>35 Ncm</p>

**Note:** Other major implant systems may require different torque values. Always consult the respective instructions for use.